

RESISTANCE THERMOMETER
Measuring insert: Interchangeable

Type:
RT-BCQ

Sheet No.
2-4 V2.1

5452-E010721V3.1




Application:

- For measuring temperatures in the food industry and the pharmaceutical, cosmetic and chemical/ technical industries

Properties:

- Resistance thermometer Pt100 and Pt1000 in acc. with IEC 60751
- Mechanical and thermal stress in acc. with DIN 43772
- Measuring insert: Interchangeable
- Parts with media contact in EN 14404 (AISI 316L)
- Withstands media temperatures of up to max 250°C
- Withstands vibrations
- Quick reaction time
- Approved by: GOST and TRCU (on request)

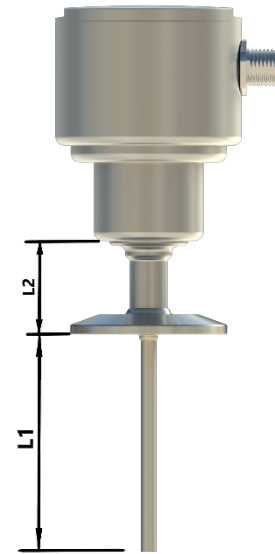

MECHANICAL SPECIFICATIONS

Protective sheath: -----
EN 1.4404 (AISI 316L) max. 850°C

Sensor diameter Ø [mm]: -----
Ø5 / Ø8
Other on request

Extension length L2 [mm]: -----
30 / 50
Other on request

Immersion length L1 [mm]: -----
20 / 35 / 50
Other on request

Process attachment: -----
3/4" APC
1 1/2" DN38, ISO2852
2" DN51, ISO2852
Special

Surface area of parts with media contact: -----
Mechanically polished <0,8 µm
Electro-polished <0,5 µm

Protection head: -----
B-SRFQ (sanitary, stainless steel, screw cap.)
Other on request

ELECTRICAL SPECIFICATIONS

---Plug (pre-mounted In Head):
M12
Harting (specify type)
Other on request

---Cable (pre-mounted in Head):
SS (Silicone-Silicone) max. 180°C
SBS (Silicone-Inner Braided-Silicone)
TBT (Teflon-Inner Braided-Teflon)
None

---Cable length [m]:

---Sensor element:
1xPt100
2xPt100
1xPt1000 (only cl. B 1/1 and cl. A)
2xPt1000 (only cl. B 1/1 and cl. A)

---Number of conductors:
2-wire (recommended only for Pt1000)
3-wire
4-wire

---Media temperature max:
+180°C
+250°C

---Tolerance in acc. with IEC 60751:
Type A DIN (i.e.±(0,15+0,002xTactual) °C)
Type B 1/1 DIN (i.e.±(0,3+0,005xTactual) °C)
Type B 1/3 DIN (i.e.±(0,1+0,0017xTactual) °C)
Type B 1/6 DIN (i.e.±(0,05+0,00083xTactual) °C)
Type B 1/10 DIN (i.e.±(0,03+0,0005xTactual) °C)

Link for further information: [Pt100 Tolerance](#)

RESISTANCE THERMOMETER
Measuring insert: Interchangeable

Type:
RT-BCQ

Sheet No.
 2-4 V2.1

5452 - E010721V3.1



Calibration:

Temperature calibration are used to verify and certify the sensor to have the correct accuracy. We can do either: "In house" or "Accredited" calibration. Accredited is certified by 3.e part. Normally we do a calibration in 3 points.

Enhanced performance services:

Cold applications (below -50°C) will influence the material and the measurement. CRYO treatment is needed to ensure a correct and working sensor down to -196°C.

A sensor will always drift over time, especially when there are high temperature fluctuations.

With "Ageing treatment" we stabilize the sensor to ensure a minimum drift over time. The benefits are long term stability, more correct measurement and easier planning of calibration periods.

Documentation:

Please order the correct documentation when ordering the sensor.



SIGNAL PROCESSING

Ceramic socket mounted in terminal head. -----

**Prepared for transmitter w/o ceramic socket. -----
 w/long leads**

Programmable head mounted transmitter-----

Measuring range min/max: -200/+850°C
 Output: 2-wire, 4-20 mA
 Min. span: 25°C
 Ambient temperature min/max: -40/+85°C

- [5333A Uninsulated for RTD](#)
- [5333D EEX Uninsulated for RTD](#)
- [5332A Uninsulated for RTD](#)
- [5332D EEX Uninsulated for RTD](#)
- [5331A Galvanic Isolated RTD / TC](#)
- [5331D EEX Galvanic Isolated RTD / TC](#)
- [5335A Hart 5 Protocol Standard](#)
- [5335D Hart 5 Protocol CSA, FM, ATEX, IECEx](#)
- [5337A Hart 5 & 7 Protocol](#)
- [5337D Hart 5 & 7 Protocol CSA, FM, ATEX, IECEx](#)



Transmitter Type:			
4 mA =	C°	20 mA =	C°

Link to further information:

[Transmitter Overview](#)

[Programmable rail mounted transmitter](#)

CALIBRATION

---Calibration:

In house (Span -33°C - +700°C)

Accredited – in laboratory (-196°C - +1200°C)

1.	Point	°C
2.	Point	°C
3.	Point	°C

More point on request

Enhanced performance services

-----Cryo treatment.

For temperature sensor under -50°C

-----Ageing:

For long term stability.
 Secure minimum drift of sensor accuracy

-----Documentation

Certificate: 3.1 Material
 Certificate of origin
 Certificate of conformity
 Certificate of GOST

Other on request