

THERMOCOUPLE THERMOMETER

Measuring insert: Fixed

Type:
TC-BM/BMC

Sheet No.
3-15 V2

5153-E010721V3.1




Application:

- Measurement of high temperatures in large ovens and channels for flue gases and air
- Field of application: Up to 1700°C (depending on thermocouple)
- Usually applied in: Tile works, refuse disposal plants and processing plants

Properties:

- Thermocouple thermometer type K, J, E, N, R, S or B in accordance with DIN IEC 60584-1
- Constructed in accordance with DS/EN 50446:2006
- Measuring insert: Fixed
- Process attachment: Adjustable flange or coupling
- Gas-proof ceramic internal tube protects thermocouple against pollution
- Outer protective sheath: Heat-proof steel or stainless acid-proof steel
- Modular construction and standard length minimizes the number of spare parts
- Can be delivered with head mounted transmitter

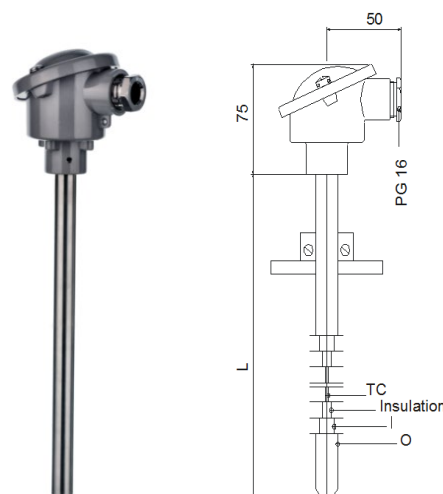

MECHANICAL SPECIFICATIONS

Protective tube O: -----

Heat-proof steel 4C54, according to DIN 50446 Special.

Internal tube according to DIN 50446: -----

Ceramics KER610
Ceramics KER799
None

Sensor diameter [mm]: -----

Ø15 mm

Nominal length L [mm]: -----

500 mm
710 mm
1000 mm
1400 mm
Other on request

Process attachment: -----

½" BSP
¾" BSP
Ø15 flange according to DIN 50446

Protection head: -----

B: (Aluminum, enameled, low cap, IP62)
BSBH: (Aluminum, enameled, high cap, IP62)
Other on request

Cable gland (pre-mounted in Head): -----

Plastic
Nickel plated brass
Stainless acid-proof steel
None

Please specify cable diameter: -----

ELECTRICAL SPECIFICATIONS

---Plug (pre-mounted in Head):

M12 (for M20)
Harting (specify type)
Other on request
None

---Cable (pre-mounted in Head):

PP (Plastic-Plastic)
SBS (Silicone-Inner Braided-Silicone)
TBT (Teflon-Inner Braided-Teflon)
Other on request
None

---Cable length [m]:

---Sensor Type:

Type T (Cu-CuNi) max. +300°C
Type J (Fe-CuNi) max. +700°C
Type E (NiCr-CuNi) max. +800°C
Type K (NiCr-Ni) max. +1150°C
Type N (NiCrSi-Ni) max. +1250°C
Type S (Pt10Rh-Pt) max +1600°C
Type R (Pt13Rh-Pt) max +1600°C
Type B (Pt30Rh-Pt6Rh) max +1700°C
Others on request

---Number of thermocouples:

1xTC
2xTC
Other on request

---Tolerance in acc. with IEC 60584-1:

Class 1 for T (i.e. $\pm 0,5^{\circ}\text{C}$ or $\pm(0,0040 \times T)$)
Class 1 for J, E, K, N (i.e. $\pm 1,5^{\circ}\text{C}$ or $\pm(0,0040 \times T)$)
Class 1 for S, R ($\pm 1,0^{\circ}\text{C}$ [$\pm 1,0^{\circ}\text{C} + (T(\text{actual}) - 1100^{\circ}\text{C})$])
Class 2 for T (i.e. $\pm 1,5^{\circ}\text{C}$ or $\pm(0,0075 \times T)$)
Class 2 for J, E, K, N (i.e. $\pm 2,5^{\circ}\text{C}$ or $\pm(0,0075 \times T)$)
Class 2 for S (i.e. $\pm 1,25^{\circ}\text{C}$ or $\pm(0,0025 \times T)$)
Class 2 for R, B (i.e. $\pm 1,5^{\circ}\text{C}$ or $\pm(0,0025 \times T)$)

Link for further information: [TC Tolerance](#)

THERMOCOUPLE THERMOMETER
Measuring insert: Interchangeable

Type:
TC-BM/BMC

Sheet No.
3-15 V2
5153-E010721V3.1




Calibration:

Temperature calibration are used to certify and verify the sensor to have the correct accuracy. We can do either: "In house" or "Accredited" calibration. Accredited is certified by 3.e part. Normally you do a calibration in 3 points.

Documentation:

Remember to order the correct documentation when ordering the sensor.

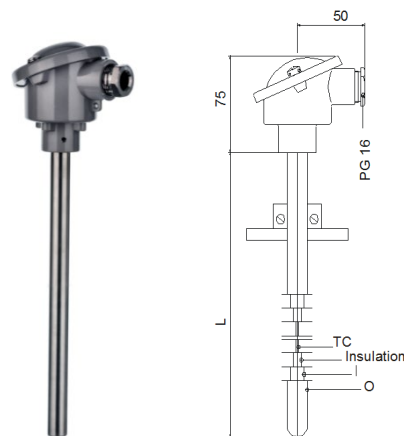

SIGNAL PROCESSING

Ceramic socket mounted in terminal head. -----

Prepared for transmitter w/o ceramic socket. -----
w/long leads

Programmable head mounted transmitter. -----

Measuring range min/max: -200/+850°C
Output: 2-wire, 4-20 mA
Min. span: 25°C
Ambient temperature min/max: -40/+85°C

[5334A Uninsulated for TC](#)

[5334D EEX Uninsulated for TC](#)

[5331A Galvanic Isolated RTD / TC](#)

[5331D EEX Galvanic Isolated RTD / TC](#)

[5335A Hart 5 Protocol Standard](#)

[5335D Hart 5 Protocol CSA, FM, ATEX, IECEx](#)

[5337A Hart 5 & 7 Protocol](#)

[5337D Hart 5 & 7 Protocol CSA, FM, ATEX, IECEx](#)




Transmitter Type:			
4 mA =	C°	20 mA =	C°

Link to further information:

[Transmitter Overview](#)

[Programmable rail mounted transmitter](#)



CALIBRATION

----Calibration:

In house (Span)
Accredited – in laboratory

1.	Point	°C
2.	Point	°C
3.	Point	°C

-----Documentation

Certificate: 3.1 Material
Certificate of origin
Certificate of conformity